




# GMA warehouse (2024 – October 1.)

	Product	Quantity
	<b>Hospital furniture etc.</b>	
1	Hospital bed	29
2	Mattress	109
3	Bedside table	30
4	Examination bed	22
6	Toilet chair	75
7	Patient lift	42
8	Patient weight	4
9	Bedsore mattress	78
	<b>Operation equipment etc.</b>	
11	Operation instruments - various	0 pallet
12	Sterilization equipment	0 pallet
13	Anesthesia tube	0 pallet
14	Anaesthesia equipment/Oxygen mask	3 pallets
15	Respirator mask	0 pallet
16	Bags for autoclave	0 pallet
17	X-ray apron	1 pallet
	<b>Nursing equipment</b>	
21	Disposable equipment-nursery	25 pallets
22	Catheter	12 pallets
23	Syringe	0 pallet
24	Bandage	0 pallet
27	Surgical gloves	5 pallets
28	Medicine glass	6 pallets
	<b>Protective equipment</b>	
31	Isolation/operation gown	62 pallets
33	Visor	66 pallets
34	Face mask	28 pallets
35	Visors with face mask	49 pallets
36	Hand sanitizer	4 pallets
37	Alcohol wipes	2 pallets
38	Wipes without alcohol	1 pallet
39	Safety glasses	1 pallet
40	Nursing aprons	0 pallets
	<b>Rehabilitation equipment etc.</b>	
41	Walker/rollator	70
42	High walker	8
43	Wheelchair	92
44	Bathing chair	119
45	Crutch and atick	105
46	Shoehorn	4 boxes
47	Heating pillow	3 pallets
48	Rehabilitation equipment (support stockings, walking frame etc.)	1 pallet
49	Walker boots/donjoys	2 pallet
50	Exercise bike	6




# GMA warehouse (2024 – October 1.)

<b>Office furniture</b>		
61	Office chair, table, bookcase etc	160
62	Tabletop	1 pallet
63	File cabinet	7
<b>Various equipment</b>		
71	Hospital/lab. clothes	6 pallets
72	Office supplies	2 pallets




# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
3		Heating cabinet		1
4.		Contrast injector Microprocessor-controlled Angiographic Injection Systems from MEDRAD MEDRAD Mark V provis MFG: 2001  Manual: <a href="https://www.scribd.com/document/440934993/medrad-mark-v-provis-service-manual">https://www.scribd.com/document/440934993/medrad-mark-v-provis-service-manual</a>	4	1
8		<i>Kinetec Performa</i> Knee CPM (Continuous Passive Motion) Machine is a state-of-the-art machine designed specifically for anatomical knee rehabilitation.  Manual: <a href="https://www.rehabmart.com/pdfs/performa_user_manual.pdf">https://www.rehabmart.com/pdfs/performa_user_manual.pdf</a>	4	1

# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
10		Spirometry Vitalograph MFG: 1996	5	5
14.		Portable Suction Unit  Mini aspeed. Battery plus  The <i>Mini-Aspeed Battery Plus</i> is a professional aspiration device specifically for post-tracheotomy patients who need numerous daily applications. MFG: 2010	4	1
20.		Intra Aortic Ballon Pump Datascope 98XT MFG: 2006 Manual: <a href="https://www.medwrench.com/documents/view/11850/datascope-98xt-service-manual-pdf">https://www.medwrench.com/documents/view/11850/datascope-98xt-service-manual-pdf</a>	2	1




# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
28.		<p>Enteral feeding pump                      Applix Smart SK                      Mfg: 2014</p>	5	13 boxes
31.		<p>Nubulizers                      Respironics                      Porta Neb                      Philips</p>	4	3
39.		<p>Centrifuge                      Hettiche                      Rotina 46                      Rotina 46S                      MFG: 2001</p>	4	2



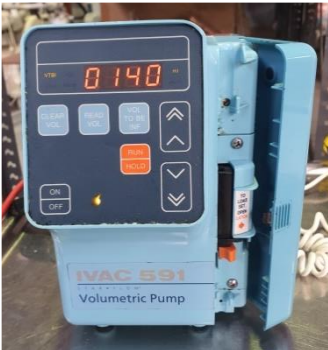
# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
41.		ENT headlight & source light Welch Allyn Solar C - 2 pcs Welch Allyn Hi-Lux SF1 – 2 pcs Lemke , Solar C – 2 pcs MFG: 2000, 2001	4	4
46.		Dentist chairs	5	6
47.		Air conditioner Cooler Tosot GPC 12 AF - K3NNA7D	5	1
49.		Sterilizer Melag 24 liters Mfg: 1996	4	1

# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
53.		<p>Nerve Stimulator - Braun</p> <p>Stimuplex HNS 11</p> <p>Stimuplex HNS 12</p> <p>Mfg: 2015</p>	5	1
54.		<p>Centrifuge</p> <p>BHG Hermle</p> <p>Z - 230</p> <p>MFG. 2001</p>		1
58.		<p>Sterilizer</p> <p>Buch og Holm</p> <p>Mfg: 2002</p>		2

# GMA warehouse (2024 – October 1.)




	Product	Description	Cat.	Quant.
60.		Infusion pump  Baxter Colleagues MFG. 2005		43
65.		Infusion pump Green Stream, VO-P ARGUS 414		5
67.		Infusion pump Volumetric Pump IVAC 591 MFG. 2008	2	7






# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
80.		Centrifuge Heraeus Biofuge Pico MFG: 1996	4	1
81.		Centrifuge Eppendorf 5415 D Mfg; 2001	4	1
89.		Microscop Leica Polyvar Richert-Jung microscope. Brightfiels & fluorescence, maybe only FITC channel Last check: 2007	4	1



# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
91.		<p>Fluoroscan Ascent</p> <p>Thermo Fisher Fluoroscan Ascent multiwell reader. Can be used for assays where multiwell plates (12-24-96) need to be evaluated for fluorescence. Has 4 distinct wavelengths. With a PC MFG: 2004</p>	4	1
93.		<p>IVF Incubator Heraeus Holten Laminair</p> <p>Incubator that regulates temperature and CO2 when connected to a source of CO2. Is used for cell culture, clinical (for instance IVF) or research purpose</p>	3	1
183		<p>Examination Lamps</p> <p>VERRE H832 S&amp;W</p> <p>Mfg: 2009</p>	5	2




# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
185		<p>Ceiling Microscope with Light source (Light optic cable partially damaged)</p> <p>Wall mounted Microscope with Light source MFG. 2002</p>	3	2
188		Cold light fountain	5	1
189		Cold light fountain	5	1




# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
196		<p>Magnilink</p> <p>Mfg: 1997</p>	5	1
197		<p>Steam Autoclave</p> <p>Melag Melaquick 12</p> <p>Mfg: 1994</p>	5	1




# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
207		Infusion pump Baxter Flo-Guard 6201 MFG: 2004	5	1
210		Oxygen generator Eclipse 3 l/min Mfg: 2014	4	1
211		Head lamp Heine Mfg: 2013	5	1




# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
213	 <p>A white Arcomed Volumed uVP2001 infusion pump. The control panel features two large red digital displays: the left one shows '3' under 'ML/H' and the right one shows '111' under 'TOTAL ML'. Below these are several control buttons and a smaller display showing '0' under 'ML INFUSED'. The brand name 'VOLUMED uVP2001' is printed on the front panel.</p>	<p>Infusion Pump Arcomed Volumed uVP2001 Mfg: 2002</p>	5	1
214	 <p>A blue Alaris Model 7131 infusion pump. It has a large green LCD screen at the top displaying '2220'. Below the screen is a numeric keypad and several function buttons. A syringe is visible in the pump's chamber on the right side.</p>	<p>Infusion pump  Alaris Model 7131  Mfg: 2004</p>	5	3
217	 <p>A white Philips patient monitor. It features a large black screen and a control panel on the right side with various buttons and a small display. The Philips logo is visible on the left side of the monitor's frame.</p>	<p>SPO2, ECG, NIBP Monitor</p>	4	1

# GMA warehouse (2024 – October 1.)




	Product	Description	Cat.	Quant.
219		SPO2, ECG, NIBP Monitor  Protocol Propaq 102 EL Mfg: 2005	4	1
221		Infusion pump Graseby Mfg: 2007		1
222		Pacemaker tester Sterling	5	1

# GMA warehouse (2024 – October 1.)



	Product	Description	Cat.	Quant.
224		Infusion pump Terumo STC-508	5	1
225		Infusion pump Terumo STC-503	5	3
226		Light source Fujinon FIL-U	4	1






# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
228		Heat cabinet for hot food	5	1
229		Vital sign monitor  Protocol Propaq Encore Mfg:2004	3	1
233		Otoscop & Oftalmoscop Welch Allyn Ref: 71940 11720 Mfg: 2013	4	1

# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
235		Microscope for eye operation Moller-Wedel Mfg: 2005	3	1
238		Halogen Light Source Universal M2-150-T Mfg: 2001	4	1


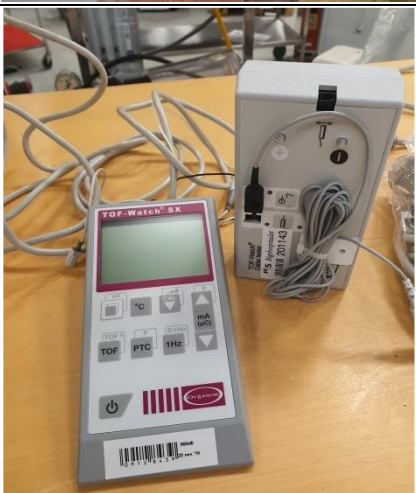

# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
239		Xenon Light Source Heine Xenon 1000 Mfg: 2008	3	1
243		Surgical ENT Drill Medtronic Xomed XPS Model: 2000	3	1
244		Blood & Fluid Warmer Barkley autocontrol Mfg: 2002	4	1




# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
245		Insufflator Lemke Vision F103 Mfg: 2007	3	1
248		Portabel Suction Unit  Laerdal	5	2
250		Light Source Olympus Highlight 2001 Mfg: 2002	4	1
251		Centrifuge Eppendorf 5702 Mfg: 2012		1





# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
253	 <p>A white rectangular water bath with a stainless steel top. The front panel features a digital display and control knobs. A red sticker is on the front. The label on the front reads 'Precision' and 'Mfg: 2000'. A handwritten note on the top right corner says '3:35 31:32 6/104' and '4-65 53:85'.</p>	<p>Water Bath</p> <p>Precision 184</p> <p>Mfg: 2000</p>	5	1
256	 <p>A handheld electronic device with a screen and several buttons. The screen displays 'TOF-Watch sx'. The device is connected to a larger white box with various ports and cables. The larger box has a label that reads 'TOF-Watch sx' and 'Mfg: 2006'.</p>	<p>TOF Watch sx Neuromuscul Stimulator</p> <p>Mfg: 2006</p>	5	15
258	 <p>A stainless steel water bath with a control panel on the left side. The control panel has a large dial and two indicator lights (red and green). The device is sitting on a yellow surface.</p>	<p>WaterBath</p> <p>Buch &amp; Holm</p> <p>Mfg: 2000</p>	4	1





# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
259		Pipets	5	30
260		Spectrometer Perkin & Elmer UV/VIS Spectrometer Lambda 2 Mfg: 2001	4	1
261		Shaker Buch & Holm Vibatron Mfg: 1997		

# GMA warehouse (2024 – October 1.)




	Product	Description	Cat.	Quant.
263		Shaker GFL 3005 Mfg: 1996	5	1
264		Hybridization Lab. Incubator Hybaid Micro-4 Mfg: 1999	4	1
265		Light Source Storz S&W Mfg: 1994	5	1
266		Electrosurgery Unit Erbe Erbotom T71D Mfg: 1995	4	1

# GMA warehouse (2024 – October 1.)



	Product	Description	Cat.	Quant.
267		Vital Signs Monitor ECG, SPO2  Mfg: 1996	5	1
268		Vacumeter	5	10
269		Microscope  Nikon SMZ-2B  Mfg: 1996	5	1
270		Intensive Care Monitor  Philips V-24C  Mfg: 1999	4	15





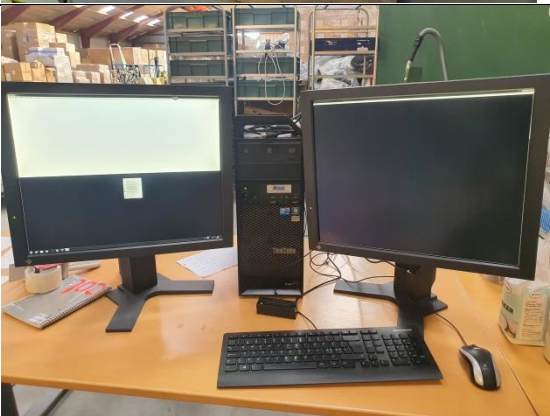
# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
271		Arthroscopy Surgical Unit Advantage Drive Systems Linvatec Hall Surgical Mfg: 2000	3	1
275		Operation Theatre Pendant Pneumatic Berlin – 3 shelvs O2,A7,A4,Vac, N2O, CO2 - Uni socket	3	1
276		ICU Pendant TRUMPF Solo Tandem O2,A4, Vac - Uni Socket	3	3

# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
277		ICU Pendant TRUMPF <b>Uniport</b> O2,A4, Vac - Uni Socket	3	3
278		ICU Pendant TRUMPF <b>Mittellast/scheplast</b> <b>Klinoport 1265</b> O2,A4, Vac - Uni Socket	3	7




# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
280		Water bath Orfit industries Suspan 2A MFG 2007	5	1
281		Washer KEN BWD 736 Mfg 2009	4	2
282		Workstation Radiology purpose	4	1




# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
284		Syringe Pump Terumo TE 312 2005	4	3
285		Drive System Conmed Linvatec D3000 Mfg 2007	3	1
286		Electrosurgical Unit Covidien Force FX Mfg 2004	4	1




# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
287		Dyonic shaver Smith & Nephew Dyonic power Mfg 2010	3	1
288		Ultra ortho suction Kebomed Lina Mfg 2006	4	1
290		X-ray incl. CEPH		


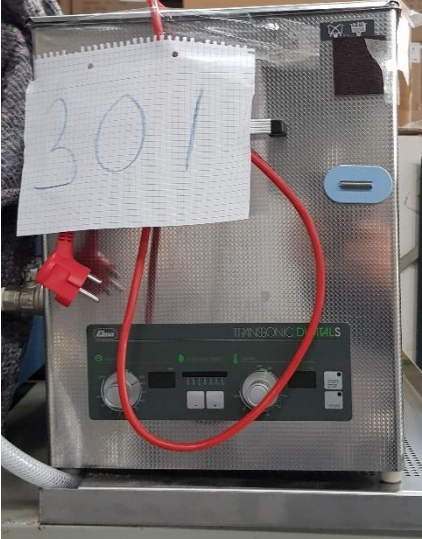
# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
291		Surgical lights		
293		Refrigerator		
294		Refrigerator		

# GMA warehouse (2024 – October 1.)

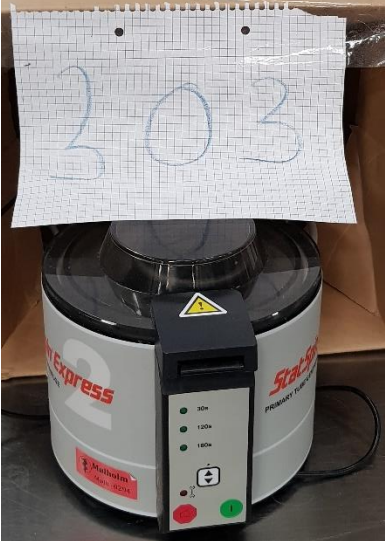

	Product	Description	Cat.	Quant.
295		Freezer/refrigerator		
297		X-ray film viewer - possible defect		
298		Suction box for laboratory or medicine		

# GMA warehouse (2024 – October 1.)

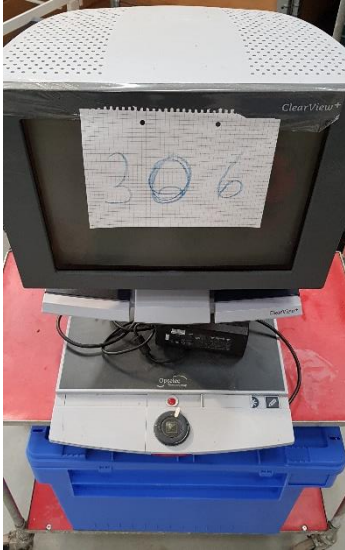

	Product	Description	Cat.	Quant.
300		Freezer		
301		Ultrasonic cleaner for dental and surgical instruments		



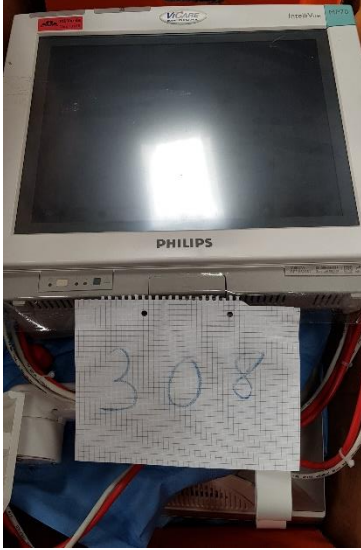

# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
303		Centrifuge		
304		Smith & Nephew 640 Image Management System for surgical pictures and videos		



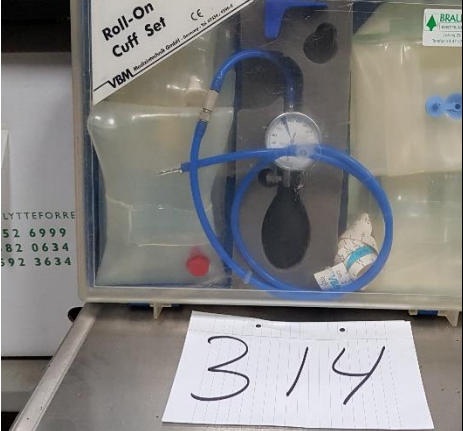

# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
306		Device for patients with visual impairment		
307		Examination lamps		



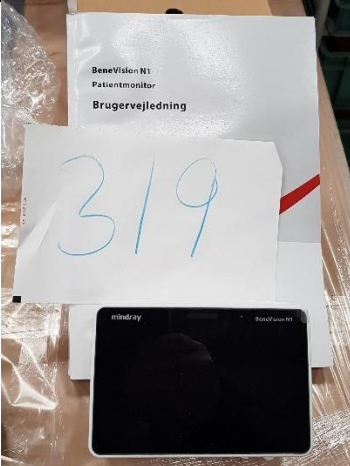
# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
308		Vital signs monitor		4
309		Cardiac assessment system for exercise testing - without screen		



# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
312		Dental chair and treatment unit		4
313		Dyonics 360 3-CCD Camera - Control Unit for handling of surgical fotos and videos (Der må være et kamera et sted, der hører til)		
314		<ul style="list-style-type: none"> <li>Roll On Cuff. Allows fast and easy blood exsanguination of an extremity (alternative to Esmarch Bandage)</li> </ul>		
316		Operation-/cliniclamp		2



# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
317		Heating box		5
318		Infusion pump		1
319		Patient monitor		2

# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
320		Audiometer		1
321		Vital signs monitor		6

# GMA warehouse (2024 – October 1.)



	Product	Description	Cat.	Quant.
323		Complete dentist x-ray equipment.		1
324		Dentist equipment		1

# GMA warehouse (2024 – October 1.)


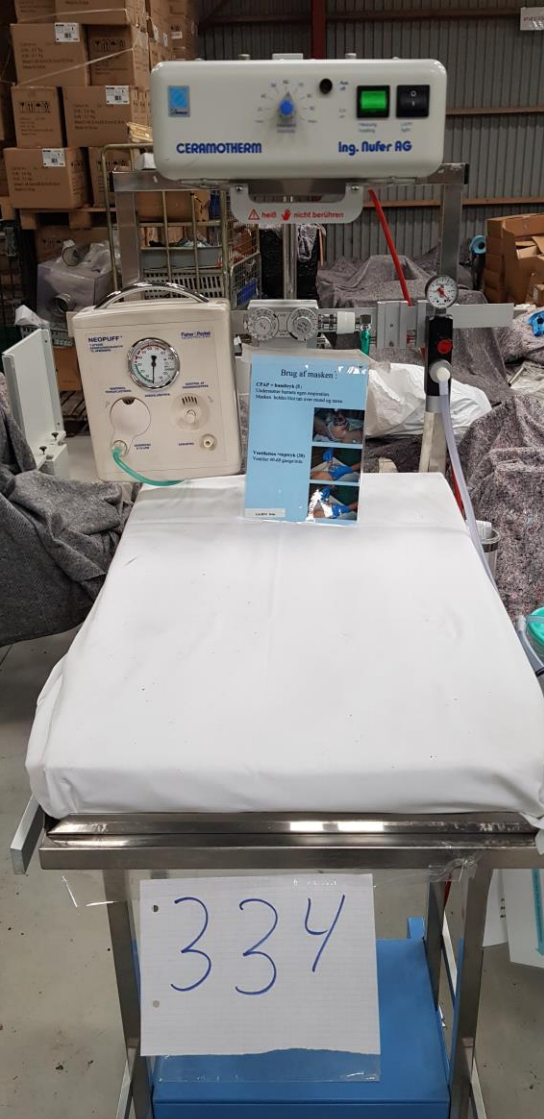
	Product	Description	Cat.	Quant.
325	 The image shows two pieces of anesthesia equipment, specifically oxygen and nitrous oxide mixers, mounted on a white cart. Each unit has a control panel with several gauges and knobs. The equipment is connected to various tubes and hoses. The background shows a warehouse setting with wooden pallets and other equipment.	Anesthesia equipment, mixer of oxygen / dinitrogen oxide		2




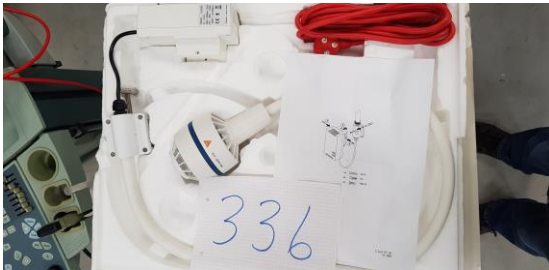
# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
327		Ultrasound		3
330		<a href="https://www.acelity.com/healthcare-professionals/global-product-catalog/catalog/abthera-open-abdomen-negative-pressure-therapy">https://www.acelity.com/healthcare-professionals/global-product-catalog/catalog/abthera-open-abdomen-negative-pressure-therapy</a>		10



# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
331		<a href="https://www.acelity.com/healthcare-professionals/global-product-catalog/catalog/cellutome-epidermal-harvesting-system">https://www.acelity.com/healthcare-professionals/global-product-catalog/catalog/cellutome-epidermal-harvesting-system</a>		10
334		<a href="https://www.weyermed.com/fileadmin/imagenes/downloads/VK_CERAMOTHERM_3000_EN_03.pdf">https://www.weyermed.com/fileadmin/imagenes/downloads/VK_CERAMOTHERM_3000_EN_03.pdf</a>  <b>CERAMOTHERM</b> radiant warmers for babies with <b>NEOPUFF</b> : a T-piece resuscitator to deliver controlled, consistent, and precise pressures – independent of operator experience. <sup>1,2</sup>  It can provide assisted respiratory breaths to neonates and infants (up to 10 kg) in the delivery room or neonatal intensive care unit		1



# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
335		Incubator		2 pcs
336		Lamps for ???		1



# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
337		Ultrasound		1
338		Centrifuge		1

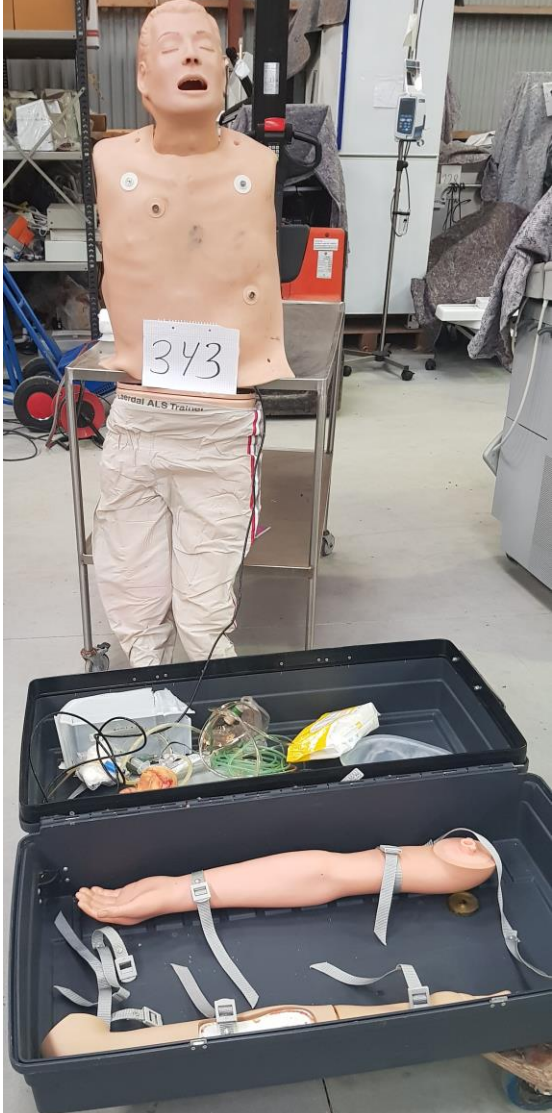
# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
339		Equipment for eye clinic		
340		Ultrasound		



# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
341		Centrifuge		
342		Centrifuge		

# GMA warehouse (2024 – October 1.)



	Product	Description	Cat.	Quant.
343		'Little Anne' – first aid		

# GMA warehouse (2024 – October 1.)



	Product	Description	Cat.	Quant.
344		Massage Chair		1
345		Shockwave therapy-system		1



# GMA warehouse (2024 – October 1.)

	Product	Description	Cat.	Quant.
346		Snellen chart		1
347		Audiometer		25

# GMA warehouse (2024 – October 1.)

<p>348</p>	<p>Type S-2010 1.8          DIN 12950 TEIL 10 : 1991          No 99106000C          Year 2001</p> <p>CE</p> <p>Manufactured by:          Histo-Holten A/S          Gydevang 17-19          DK-3450 Allerød          Denmark</p> <p>A 2,6          V 230~          Hz 50          W 600</p> <p>CONTROLLED 010209          NEXT CHECK UP 020209          SIGN B.D.</p> 	<p>Laboratory bench</p>		<p>1</p>
<p>350</p>		<p>Feeding pump</p>		<p>72</p>